

Now sold under the
Thermo Scientific brand

Thermo
SCIENTIFIC

Ion Chromatography: A Versatile Technique for the Analysis of Beer

INTRODUCTION

Ion chromatography is an efficient technique for the analysis and quantification of ions in solution. Although there are several techniques that have been used for the analysis of beer — including gas chromatography, HPLC, enzyme-based methods, and wet chemical methods — ion chromatography is rapidly becoming the method of choice.

The compounds of interest for the beer industry range — from inorganic ions, organic acids, and hop bittering principles that contribute to the overall taste and bitterness of the beverage — to proteins, carbohydrates, and alcohols that are monitored to determine the extent of fermentation. The finished beer product may be analyzed to determine the concentration of added preservatives and colorants, in addition to ensuring manufacturing authenticity.

The first step in the beer making process involves soaking barley, and sometimes other grains, in warm water. Enzymes present in the barley break down starch from the grains, producing mostly glucose, maltose, and other oligo- and polysaccharides. This process is called mashing, and the resulting solution is called sweet wort. The sweet wort is then treated with hops, thereby producing hopped wort. Yeast is added and the smaller saccharides are fermented to produce alcohol. Because of the different concentrations, chemical behavior, and molecular mass ranges of the various components in beer, their isolation and determination can be difficult. Ion chromatography, using polymer-based resins, provides a means to monitor many of these important compounds during the brewing process and in the final product.

This application note describes the use of ion-exchange or ion-exclusion chromatography for the determination of five classes of compounds of interest to the brewing industry, including: carbohydrates, alcohols, organic acids, inorganic anions, and inorganic cations. One of two forms of electrochemical detection is used, pulsed amperometry or conductivity detection.

EQUIPMENT

A Dionex chromatographic system consisting of:

- Gradient Pump
- Chromatography Enclosure
- Electrochemical Detector with pulsed amperometry and conductivity modes
- Eluent Organizer

PeakNet Chromatography Workstation

REAGENTS AND STANDARDS

Deionized water, 17.8 M Ω -cm or better

Carbohydrate Analysis

- Sodium acetate (Sigma)
- Sodium hydroxide solution, 50% (w/w) (Fisher Scientific)

Anion Analysis

- Sodium hydroxide solution, 50% (w/w) (Fisher Scientific)
- Methanol (EM Science)

Alcohol Analysis

Perchloric acid (Fisher Scientific)

Cation Analysis

Methanesulfonic acid (Fluka Chemika-BioChemika)

Organic Acid Analysis

0.1 M Tetrabutylammonium hydroxide (TBAOH)
(Dionex P/N 39602)

Heptafluorobutyric acid (Fluka Chemika-BioChemika)

PREPARATION OF SOLUTIONS AND REAGENTS

1.00 M Sodium Acetate

Weigh out 82.0 g of anhydrous sodium acetate and place into a 1-L volumetric flask. Add approximately 600 mL of 17.8 M Ω -cm deionized water and swirl to dissolve.

When the salt has dissolved completely, fill up to the mark with 17.8 M Ω -cm deionized water. Filter the resulting solution through a 0.2- μ m filter.

500 mM Sodium Hydroxide

Weigh 974 g (974 mL) of 17.8 M Ω -cm deionized water into an eluent reservoir bottle. Degas the water for approximately 10 minutes. Tare the bottle on the balance and add 40.0 g (26.2 mL) of 50% (w/w) sodium hydroxide directly to the bottle. Quickly transfer the eluent bottle to the instrument and pressurize it with helium.

100 mM Sodium Hydroxide

Weigh 992 g (992 mL) of 17.8 M Ω -cm deionized water into an eluent reservoir bottle. Degas the water for approximately 10 minutes. Tare the bottle on the balance and add 8.00 g (5.25 mL) of 50% (w/w) sodium hydroxide directly to the bottle. Quickly transfer the eluent bottle to the instrument and pressurize it with helium.

1.00 mM Sodium Hydroxide

Place 990 g (990 mL) of 17.8 M Ω -cm deionized water into an eluent reservoir bottle. Degas the water for approximately 10 minutes. Pipette 10.0 mL of the 100 mM sodium hydroxide solution directly into the bottle. Quickly transfer the eluent bottle to the instrument and pressurize it with helium.

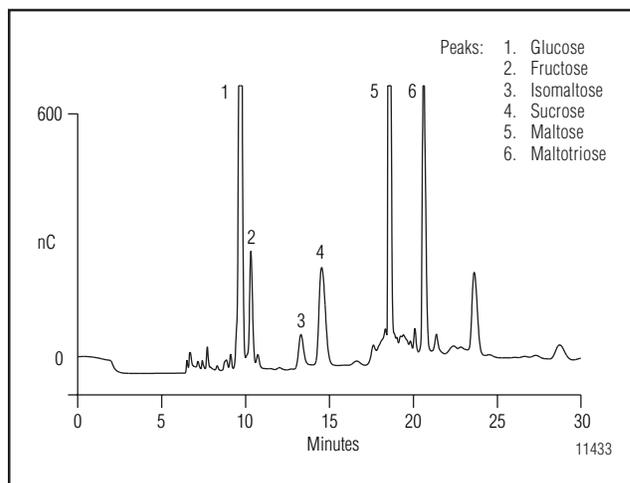


Figure 1 Separation of fermentable sugars in wort by ion-exchange chromatography with pulsed amperometric detection. Experimental conditions are listed in Table 2. The sample was diluted 1:10 before injection.

100 mM Methanesulfonic Acid

Weigh out 9.61 g of methanesulfonic acid (MSA). Carefully add this amount to a 1-L volumetric flask containing about 500 mL of deionized water. Dilute to the mark and mix thoroughly.

100 mM Perchloric Acid

Dilute 8.60 mL of perchloric acid into 992 mL of 17.8 M Ω -cm deionized water.

0.8 mM Heptafluorobutyric Acid

Heptafluorobutyric acid (perfluorobutyric acid) is supplied by FLUKA in 10.0-mL bottles. Dilute the entire contents of one 10.0-mL bottle in 1.00 L to obtain a 77.2 mM stock solution. Dilute 10.4 g of the stock solution in 1.00 L to obtain the 0.800 mM working eluent.

5 mM Tetrabutylammonium Hydroxide

Dilute 50 mL of the Dionex 0.1 M TBAOH ion-pairing reagent (P/N 35360) to 1 L with 17.8 M Ω -cm deionized water. Prepare several liters of the regenerant.

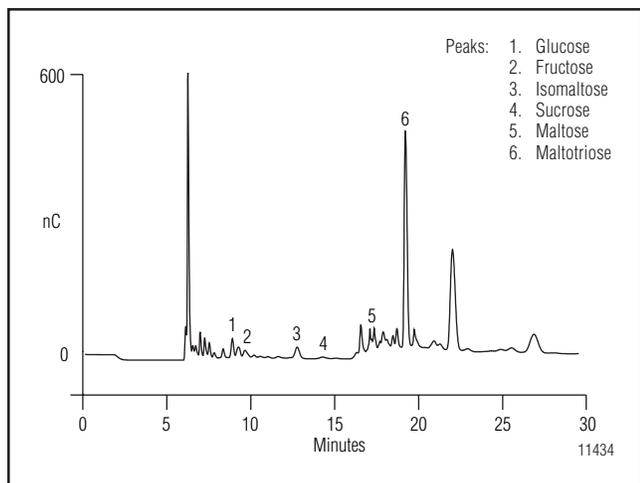


Figure 2 Separation of mono-, di-, and trisaccharides in an American beer by ion-exchange chromatography with pulsed amperometric detection. Experimental conditions are listed in Table 2. The sample was diluted 1:10 before injection.

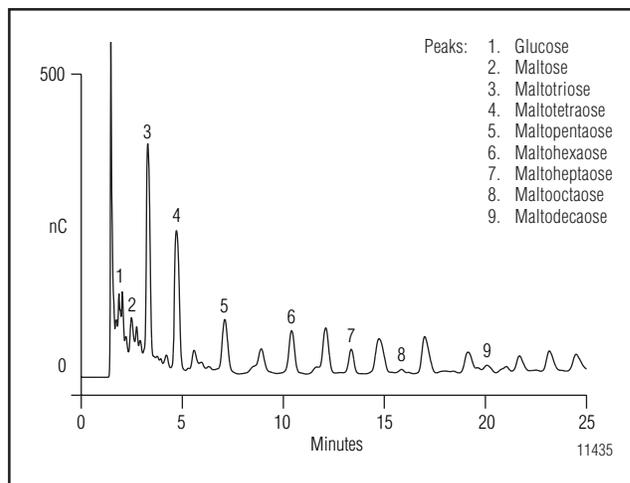


Figure 3 Separation of malto-oligosaccharides in an American beer by ion-exchange chromatography with pulsed amperometric detection. Experimental conditions are listed in Table 3. The sample was diluted 1:10 before injection.

RESULTS AND DISCUSSION

Carbohydrate Analysis

Carbohydrates and other species containing hydroxyl functional groups can be detected by measuring the current caused by their oxidation at a gold electrode. A repeating sequence of three applied potentials is used first to oxidize the carbohydrates, and then to clean the electrode of the products of the oxidation reaction by applying a large positive and then a negative potential. This sequence is repeated once every second to eliminate electrode fouling and thereby to ensure a reproducible response. Unless this sequence is performed, the peak heights will steadily decrease as the electrode surface becomes fouled. For the chromatograms shown in Figures 1, 2, and 3, the electrochemical detector was programmed with the waveform shown in Table 1. Integration was performed from 0.2 to 0.4 seconds. Other waveforms that have been developed and tested are described in *Technical Note 21, "Optimal Settings for Pulsed Amperometric Detection of Carbohydrates Using Dionex Pulsed Electrochemical and Amperometric Detectors,"* and may provide superior results in some cases.

Because carbohydrates have pK_a s between 12 and 14, they can be separated as anions by ion-exchange chromatography. To drive the oxidation reaction at the working electrode, the eluent must be above pH 12, thus the resins in the Dionex CarboPac™ columns are polymer-based for stability and durability in the pH range 0–14. Using a hydroxide gradient, the sugars are separated on the CarboPac PA1 in the following order: monosaccharides,

Table 1 ED40 waveform for the analysis of carbohydrates by ion chromatography using a gold electrode

Time (s)	Potential (V)
0.00	0.05
0.40	0.05
0.41	0.75
0.60	0.75
0.61	-0.15
1.00	-0.15

Table 2 Experimental conditions for the separation of mono-, di-, and trisaccharides in beer and wort by ion-exchange chromatography

Column:	CarboPac PA1			
Eluent 1:	Deionized water			
Eluent 2:	500 mM Sodium hydroxide			
Gradient:	Time	E1	E2	Comments
	Initial	99	1	Reequilibrate
	5.00	99	1	Inject
	6.00	99	1	Back to Load
	20.00	91	9	
	45.00	0	100	
	50.00	0	100	
Flow Rate:	1.0 mL/min			
Inj. Volume:	10 μ L			
Detection:	Pulsed amperometry, gold electrode (see Table 1 for waveform)			

disaccharides, and trisaccharides. The experimental conditions used for the separations shown in Figures 1 and 2 are presented in Table 2.

The carbohydrates of most importance to the brewing industry are the fermentable sugars. In general, saccharides larger than DP3 are not fermentable; however, they will contribute to the caloric value as well as to the overall flavor of the beer and its ability to form a head. Figure 1 shows the separation of fermentable sugars (\leq DP3) in a hopped wort sample. These are the sugars that are converted by yeast to alcohol. If this figure is compared with the separation shown in Figure 2, the difference between the finished beer and a beer during production is evident. As expected, the concentration of fermentable sugars is greater in the wort than in the final beer product.

The complex sugars, starches, and dextrans, which are broken down by enzymes to produce a wort of high fermentability, are built up from glucose sub-units. Maltose is the simplest of the complex sugars and is formed by two glucose molecules joined together by an α -1,4 linkage. Following convention, chains are named according to the number of glucose units that have been incorporated. Thus, maltotetraose (DP4), for example, is a chain of four glucose units linked together by α -1,4 linkages.

Figure 3 shows the separation of maltose oligosaccharides in beer from DP3 to DP10, using the CarboPac PA-100. Excellent resolution of maltose oligomers up to DP15 is possible, allowing for rapid profiling. As indicated in the experimental conditions listed in Table 3, the eluent contained sodium acetate in addition to sodium hydroxide. The sodium acetate increases the eluent strength, which reduces the retention time of the oligosaccharides. Separation is possible in the absence of sodium acetate, but the run times are prohibitively long.

Alcohol Analysis

Usually, the only two alcohols present in high concentrations in beer are ethanol and glycerol. Glycerol is an important component in beer; it has a considerable effect on flavor and is sweeter than glucose. Ethanol and glycerol can be separated by ion-exclusion chromatography, then detected with pulsed amperometry using the waveform described in Table 4 with integration performed from 0.05 to 0.25 seconds.

Table 3 Experimental conditions for the separation of oligosaccharides in beer using the CarboPac PA-100

Column:	CarboPac PA-100				
Eluent 1:	Deionized water				
Eluent 2:	500 mM Sodium hydroxide				
Eluent 3:	1 M Sodium acetate				
Gradient:	Time	E1	E2	E3	Comments
	Initial	57	33	10	Reequilibrate
	1.50	57	33	10	Inject
	6.50	57	33	10	Gradient Start
	31.50	42	33	25	Gradient End
Flow Rate:	1.0 mL/min				
Inj. Volume:	10 μ L				
Detection:	Pulsed amperometry, gold electrode (see Table 1 for waveform)				

Table 4 ED40 waveform for the analysis of alcohols by ion-exclusion chromatography using a platinum electrode

Time (s)	Potential (V)
0.00	0.30
0.05	0.30
0.25	0.30
0.26	1.25
0.60	1.25
0.61	0.10
1.00	0.10

Table 5 Experimental conditions used for the separation of glycerol and ethanol by ion-exclusion chromatography using the IonPac ICE-AS6 column

Column:	IonPac [®] ICE-AS6
Eluent:	100 mM Perchloric acid
Flow Rate:	2.0 mL/min
Inj. Volume:	10 μ L
Detection:	Pulsed amperometry, platinum electrode (see Table 4 for waveform)

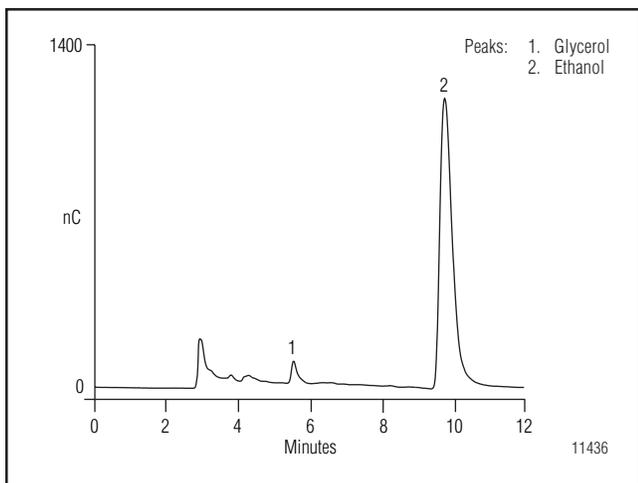


Figure 4 Separation of glycerol and ethanol in an American beer by ion-exclusion chromatography with pulsed amperometric detection. Experimental conditions as listed in Table 5. The sample was diluted 1:10 before injection.

The IonPac ICE-AS6 column is an ion-exclusion column that successfully separates alcohols. The experimental conditions used for the separation of glycerol and ethanol are listed in Table 5. Figure 4 shows the separation of ethanol and glycerol in beer by ion-exclusion chromatography using pulsed amperometric detection with a platinum electrode.

Organic Acid Analysis

The measurement of organic acids, in all phases of beer production, can be used to help track metabolic products of fermentation and to correlate beer flavor trends. One way to separate organic acids is with ion-exclusion chromatography using suppressed conductivity detection. The IonPac ICE-AS6 column is an ion-exclusion column designed for the efficient separation of low molecular weight aliphatic organic acids including hydroxy-substituted organic acids, in addition to species such as aliphatic alcohols and glycols. Using this separation mechanism, weakly ionized species are separated based on differences in their pK_a s. Strong inorganic acid anions are not retained by the stationary phase and elute in the void volume of the column. The standard eluent for use with the IonPac ICE-AS6 is 0.4 mM heptafluorobutyric acid (perfluorobutyric acid). Other monoprotic acids can be used; however, the background conductivity will be higher. The experimental conditions are listed in Table 6.

Table 6 Experimental conditions for the separation of organic acids in beer by ion-exclusion chromatography using the IonPac ICE-AS6 column

Column:	IonPac ICE-AS6
Eluent:	0.8 mM Heptafluorobutyric acid
Flow Rate:	1.0 mL/min
Inj. Volume:	25 μ L
Detection:	Suppressed conductivity, AMMS™-ICE
Regenerant:	5 mM Tetrabutylammonium hydroxide at 5 mL/min

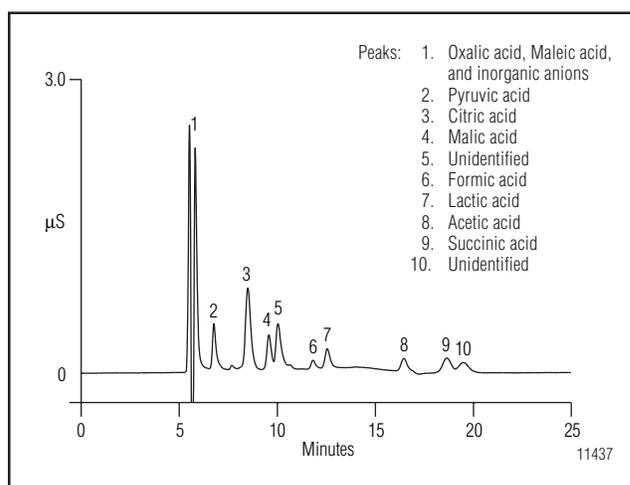


Figure 5 Separation of organic acids in a British stout. Experimental conditions are listed in Table 5. The sample was diluted 1:40 before injection.

Figure 5 shows the separation of a series of organic acids in a stout. The sample was degassed and diluted 1:40 prior to injection. Oxalic and maleic acids are eluted on either side of the ‘water dip,’ masked by strong acid anions such as fluoride and chloride. Pyruvate, citrate, malate, formate, lactate, acetate, and succinate, however, are all baseline resolved. The presence of acetate may provide evidence of oxidation, while pyruvic acid is present as an intermediate product in the conversion of glucose to alcohol. Lactate is produced by lactic acid bacteria that convert glucose and other sugars to lactic acid, so it is kept to a minimum in most beers. A few unidentified peaks are also resolved.

Inorganic Anions

Inorganic anions are introduced into beer from the brewing water and have an important impact on the flavor of beer. Thus, the water can be monitored by ion chromatography to ensure purity and consistency. Despite the deliberate addition of high levels of some anions such as sulfate (Burtonization), excessive amounts of sulfate and chloride, for example, can have a detrimental effect on the flavor of the beer. In addition, high concentrations of other anions such as nitrate (if it is converted to nitrite) can harm the yeast during the fermentation process. Therefore, monitoring the anion profile is an important quality control step in the brewing industry.

Inorganic anions are separated by anion-exchange chromatography and monitored by suppressed conductivity detection; Table 7 lists the experimental conditions. When performing gradient elution on the IonPac AS11 column, a hydroxide eluent system is used instead of a carbonate eluent because of the low background conductivity of hydroxide. An Anion Trap Column (ATC) should be installed between the gradient pump and the injection valve to minimize baseline shifts resulting from the elution of anionic contaminants in the eluent.

Figure 6 shows the simultaneous separation of a mixture of inorganic and organic anions in an American ale using the IonPac AS11 column. The sample was degassed and diluted 1:40 prior to injection. The sodium hydroxide concentration in Eluent 2 is weak enough that not only is fluoride eluted after the void, but several weakly retained monovalent organic acids are also resolved. The addition of methanol to the eluent modifies the selectivity of the column for the more hydrophobic anions, thus allowing resolution between succinate and malate and also between tartrate and maleate, which would otherwise coelute. Thus, using the conditions described in Table 6, it is possible to separate not only the strong acid anions, but also a variety of weak organic acids. To obtain a flat baseline for this chromatogram, the baseline subtraction option in the PeakNet software was used. Reproducibility for this method is on the order of 0.5% or better for retention times and 2% or better for peak areas with good linearity ($r^2=0.999$) over the range tested (1.5 orders of magnitude).

Table 7 Experimental conditions for the separation of inorganic anions in beer using the IonPac AS11 column

Column:	IonPac AS11 Analytical (4 mm) IonPac AG11 Guard (4 mm) IonPac ATC-1 Anion Trap				
Eluent 1:	Deionized water				
Eluent 2:	1 mM Sodium hydroxide				
Eluent 3:	100 mM Sodium hydroxide				
Eluent 4:	Methanol				
Gradient:	Time	E1	E2	E3	E4
	Initial	80	20	—	—
	3.00	80	20	—	—
	5.00	66	20	—	14
	18.00	42	—	38	20
	18.01	80	20	—	—
Flow Rate:	2 mL/min				
Inj. Volume:	25 μ L				
Detection:	Suppressed conductivity, ASRS™, AutoSuppression™ recycle mode				

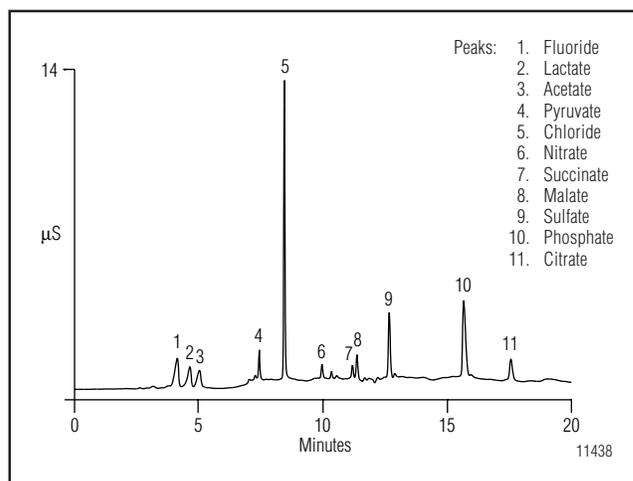


Figure 6 Separation of inorganic anions and organic acids in an American ale by ion-exchange chromatography. Experimental conditions are listed in Table 6. The sample was diluted 1:40 before injection.

Table 8 Experimental conditions for the separation of inorganic cations in beer using the IonPac CS12 column

Column:	IonPac CS12 Analytical (4 mm) IonPac CG12 Guard (4 mm) IonPac CTC-1 Cation Trap				
Eluent 1:	Deionized water				
Eluent 2:	100 mM Methanesulfonic acid				
Gradient:	Time	E1	E2	E3	E4
	Initial	84	16	—	—
	5.00	84	16	—	—
	5.01	60	40	—	—
	10.00	60	40	—	—
	10.01	84	16	—	—
Flow Rate:	1.0 mL/min				
Inj. Volume:	25 μ L				
Detection:	Suppressed conductivity, CSRS™, AutoSuppression recycle mode				

The first inorganic anion to be eluted is fluoride, which is often added to municipal water supplies to prevent tooth decay and is harmless for brewing purposes. Chloride is eluted next, and at levels above 250 mg/L it has been found to enhance the sweetness of beer. However, it may also hamper yeast flocculation. Nitrate was once thought of as a problem in the brewing process, but it has since been discovered that it is the nitrite produced from nitrate that affects yeast metabolism to cause weak and incomplete fermentation. Sulfate is found naturally in water but imparts a sharp, dry edge to well hopped beers and is therefore kept to a minimum. Finally, phosphate is present in the malt and buffers the mash at a slightly acidic pH.

Inorganic Cations

As is the case with the inorganic anions, most of the inorganic cations are introduced into the beer from the water supply. The four most abundant cations in beer are sodium, potassium, calcium, and magnesium. Some of these cations affect the pH of the mash, while others affect the flavor of the beer. Other metals such as lead, copper, and zinc are also monitored to ensure their absence since most of them are poisonous at any significant level. This application note focuses on the alkali and alkaline earth metals.

Inorganic cations are separated by ion-exchange chromatography and monitored by suppressed conductivity detection, as described in Table 8. The gradient

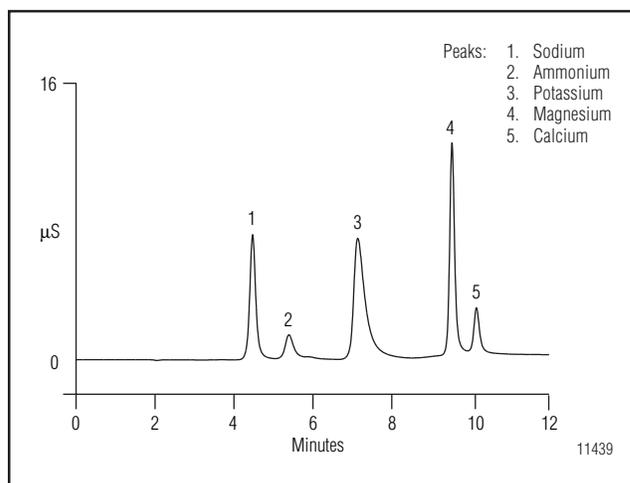


Figure 7 Separation of inorganic cations in a 1:40 dilution of an American lager by ion-exchange chromatography using the IonPac CS12 column. Experimental conditions are listed in Table 8.

allows for the separation of barium and strontium in addition to the five cations shown in Figure 7. A step change at 5 minutes from the weak eluent to a stronger eluent allows for the elution of sharp peaks for the divalent cations. The reproducibility of this method is on the order of 0.5% or better for retention times and 2% or better for peak areas. Linearity is good over the range tested (2 orders of magnitude) with a coefficient of determination, $r^2 = 0.999$ or better, for all analytes except ammonium. If it is not important to monitor for barium or strontium, the conditions can be changed to allow for isocratic elution of the five cations shown in Figure 7 (≤ 10 minutes). If isocratic elution is desired, then the concentration eluent should be 20 mM methanesulfonic acid.

Figure 7 shows the separation of the main cations in beer using the IonPac CS12 column. The sample was degassed and diluted 1:40 prior to injection. Sodium was the first peak to be eluted. At a concentration of 75–150 mg/L, it gives a round smoothness to the beer when combined with chloride. If too much sulfate is present, however, sodium gives an unpleasant harshness to the flavor. Potassium is the next metal to be eluted, and like sodium it can impart a slightly salty flavor to the beer. It also inhibits the action of certain enzymes in mash. Magnesium is an important nutrient for yeast at levels around 10–20 mg/L, but imparts a sharp, bitter-sour flavor at levels much higher than 20 mg/L. Calcium is perhaps the most important

metal, since it reacts with phosphate in the malt to lower the pH of the mash and wort. It also assists enzyme action, but has no effect on the flavor of the beer.

CONCLUSION

Carbohydrates, alcohols, organic acids, and inorganic anions and cations can all be separated on various ion-exchange or ion-exclusion columns and detected by pulsed amperometric or suppressed conductivity detection.

Although many of these constituents can be determined individually using unrelated analytical techniques, reduced analysis time and equipment costs can be realized by using one instrument with multi-species capability. Ion chromatography is a versatile technique that meets many of the analytical requirements of the beer making process.

LIST OF SUPPLIERS

EM Science, P.O. Box 70, 480 Democrat Road,
Gibbstown, New Jersey, 08027, USA,
1-800-222-0342.

Fisher Scientific, 711 Forbes Ave., Pittsburgh,
Pennsylvania, 15219-4785, USA, 1-800-766-7000.

Fluka Chemika-BioChemika, Fluka Chemie AG,
Industriestrasse 25, CH-9471 Buchs, Switzerland, +81
755 25 11.

Sigma Chemical Company, P.O. Box 14508, St. Louis,
Missouri, 63178, USA, 1-800-325-3010.

AMMS, CSRS, ASRS, and CarboPac are trademarks and IonPac is a registered trademark of Dionex Corporation.

 Printed on recycled and recyclable paper with soy-based ink.

Dionex Corporation
1228 Titan Way
P.O. Box 3603
Sunnyvale, CA
94088-3603
(408) 737-0700

Dionex Corporation
Salt Lake City Technical Center
1515 West 2200 South, Suite A
Sunnyvale, CA
84119-1484
(801) 972-9292

Dionex U.S. Regional Offices
Sunnyvale, CA (408) 737-8522
Westmont, IL (630) 789-3660
Houston, TX (281) 847-5652
Smyrna, GA (770) 432-8100
Marlton, NJ (609) 596-0600

Dionex International Subsidiaries
Austria (431) 616 51 25 Belgium (015) 203800 Canada (905) 844-9650 France 01 39 46 08 40 Germany (06126) 991-0
Italy (6) 66030052 Japan (06) 885-1213 The Netherlands (076) 57 14 800 Switzerland (062) 205 99 66 United Kingdom (01276) 691722
* Designed, developed, and manufactured under an NSAI registered ISO 9001 Quality System.
<http://www.dionex.com>

