

Now sold under the  
Thermo Scientific brand

**Thermo**  
SCIENTIFIC

# Determination of Trace Concentrations of Chlorite, Bromate, and Chlorate in Bottled Natural Mineral Waters

## **INTRODUCTION**

Bottled water has been one of the fastest growing beverage markets in the last five to ten years. Global consumption approached 41 billion gallons in 2004, an increase of 6.5% from 2003.<sup>1</sup> The bottled water industry markets to health conscious consumers as an alternative not only to tap water, but also to carbonated soft drinks and juice drinks.<sup>1</sup> Regardless of whether the water is delivered from a local municipality or is prepackaged in a bottle, the consumption of safe and reliable drinking water is essential to maintain a healthy lifestyle.

Bottled water must be disinfected to remove pathogenic microorganisms and ensure it is safe for human consumption. Water companies prefer ozone as a disinfectant because it is one of the most effective treatments available, it does not leave a taste, and there is no residual disinfectant in the bottled water.<sup>2,3</sup> Some bottlers, however, use ultraviolet light or chlorine dioxide as alternative treatment methods.<sup>2</sup> Reactions between disinfectants and natural organic and inorganic matter in the source water can result in the production of undesirable disinfection byproducts (DBPs), such as chlorite, bromate, and trihalomethanes, that are potentially harmful to humans.<sup>4</sup> Bromate, for example, can be formed by ozonation of water containing naturally occurring bromide, or may be present as an impurity in sodium hypochlorite used for treatment.<sup>5</sup>

Results from toxicological studies led the International Agency for Research on Cancer to conclude that bromate is a potential human carcinogen, even at low

$\mu\text{g/L}$  (ppb) concentrations.<sup>6</sup> The World Health Organization (WHO) estimated excess lifetime cancer risks of  $10^{-4}$ ,  $10^{-5}$ , and  $10^{-6}$  for drinking water containing bromate at 20, 2, and  $0.2 \mu\text{g/L}$ , respectively.<sup>9</sup> The U.S. EPA,<sup>7</sup> European Commission,<sup>8</sup> and the WHO<sup>9</sup> set a maximum permissible limit of  $10 \mu\text{g/L}$  bromate in tap water. The U.S. FDA<sup>10</sup> adopted the same regulatory limit for bottled water. In Europe, natural mineral waters and spring waters treated by ozonation have a maximum permissible limit of  $3 \mu\text{g/L}$  bromate.<sup>11</sup>

Traditionally, ion chromatography (IC) with suppressed conductivity detection has been used for determination of bromate and other DBPs in drinking water, as described in EPA Method 300.1.<sup>12</sup> This method describes the use of a high-capacity IonPac AS9-HC column with a carbonate eluent and large loop injection to achieve a method detection limit (MDL) of  $1.4 \mu\text{g/L}$  bromate. In early 2006, the U.S. EPA enacted stage 2 of the disinfectants/disinfection byproducts (D/DBP) rule, maintaining the maximum permissible limit for bromate but adding three additional analytical methods to further improve the selectivity and sensitivity for bromate.<sup>13</sup> U.S. EPA Methods 317.0 and 326.0 combine suppressed conductivity detection and absorbance detection after postcolumn addition to achieve bromate MDLs less than  $0.2 \mu\text{g/L}$ .<sup>14,15</sup> IC coupled to inductively coupled plasma mass spectrometry has also been demonstrated for the determination of low concentrations of bromate in environmental waters, permitting a bromate MDL of  $0.3 \mu\text{g/L}$ .<sup>16</sup>

A high-capacity IonPac® AS19 column with an electrolytically generated hydroxide eluent, large loop injection, and suppressed conductivity detection can achieve a calculated bromate MDL of 0.34 µg/L.<sup>17</sup> Absorbance detection after postcolumn addition can reduce this MDL to less than 0.2 µg/L, using EPA Methods 317.0 and 326.0.<sup>18,19</sup> In this application note, we compare the IonPac AS19 using an electrolytically generated hydroxide eluent to the IonPac AS23 column using an electrolytically generated carbonate/bicarbonate eluent for the determination of chlorite, bromate, and chlorate in natural mineral waters. We compare the linearity, method detection limits, precisions, and recovery for three mineral waters obtained from three European countries to determine whether these columns have the sensitivity required to meet current EPA and EU requirements.

### **EQUIPMENT**

A Dionex ICS-2000 Reagent-Free™ Ion Chromatography (RFIC™) system was used in this work. The ICS-2000 is an integrated ion chromatograph and consists of:

- Eluent generator
- Pump with in-line vacuum degas
- Column heater
- Hydroxide system:
  - EluGen® EGC II KOH cartridge (Dionex P/N 058900)
- CR-ATC (Dionex P/N 060477)
- Carbonate system:
  - EluGen EGC II K<sub>2</sub>CO<sub>3</sub> cartridge (Dionex P/N 058904)
- EPM Electrolytic pH Modifier to generate the carbonate/bicarbonate eluent (Dionex P/N 063175)
- EGC Carbonate Mixer (Dionex P/N 079943)
- Two 4-L plastic bottle assemblies (for external water mode of suppression)
- AS Autosampler
- Chromeleon® Chromatography Management Software

### **REAGENTS AND STANDARDS**

- Deionized water, type I reagent grade, 18 MΩ-cm resistivity or better
- Sodium chlorite (NaClO<sub>2</sub>, Fluka 71388, 80% pure)
- Sodium bromate (NaBrO<sub>3</sub>, EM SX 03785-1)
- Sodium chlorate (NaClO<sub>3</sub>, Fluka 71370)

### **CONDITIONS**

- Columns: (A) IonPac AS19 Analytical, 4 x 250 mm (Dionex P/N 062885) IonPac AG19 Guard, 4 x 50 mm (Dionex P/N 062887)  
(B) IonPac AS23 Analytical, 4 x 250 mm (Dionex P/N 064149) IonPac AG23 Guard, 4 x 50 mm (Dionex P/N 064147)
- Eluent: (A) 10 mM KOH from 0–10 min, 10–45 mM from 10–25 min, 45 mM from 25–30 min\*  
(B) 4.5 mM K<sub>2</sub>CO<sub>3</sub>/0.8 mM KHCO<sub>3</sub>
- Eluent Source: (A) EGC II KOH with CR-ATC  
(B) EGC II K<sub>2</sub>CO<sub>3</sub> with EPM
- Flow Rate: 1.0 mL/min
- Temperature: 30 °C
- Injection: 250 µL
- Detection: (A) Suppressed conductivity, ASRS® ULTRA II, 4 mm (Dionex P/N 061561) AutoSuppression® recycle mode 130 mA current  
(B) Suppressed conductivity, ASRS ULTRA II, 4 mm AutoSuppression external water mode 25 mA current
- CRD: (A) 4-mm format (P/N 062983)
- Background
- Conductance: (A) <1 µS  
(B) 18–20 µS
- System
- Backpressure: ~2200 psi
- Run Time: 30 min

\*Method returns to 10 mM KOH for 3 min prior to injection.

### **PREPARATION OF SOLUTIONS AND REAGENTS**

#### **Eluent Solution for the AS23 Column**

#### **4.5 mM Carbonate/0.8 mM Bicarbonate**

Generate the carbonate/bicarbonate eluent on-line by pumping high quality deionized water (18 MΩ-cm resistivity or better) through the EluGen EGC II K<sub>2</sub>CO<sub>3</sub> Cartridge and EPM. Chromeleon will track the amount of eluent used and calculate the remaining lifetime.

Alternatively, prepare the eluent solution by adding 10 mL of the AS23 Eluent Concentrate (Dionex P/N 064161) to a 1-L volumetric flask containing

approximately 700 mL of degassed deionized water. Bring to volume and mix thoroughly. The 0.45 M sodium carbonate/0.08 M sodium bicarbonate concentrate can also be prepared from the salts by combining 47.7 g sodium carbonate (MW=106 g/mole) and 6.72 g sodium bicarbonate (MW=84 g/mole) in a 1-L volumetric flask containing approximately 700 mL of degassed deionized water. Bring to volume and mix thoroughly.

### Stock Standard Solutions

Prepare 1000 mg/L stock standard solutions of chlorite, bromate, and chlorate by dissolving 0.1676 g, 0.1180 g, and 0.1275 g, respectively, of the corresponding sodium salts in separate 100 mL volumetric flasks of DI water.

### Calibration Standard Solutions

Prepare a secondary stock solution containing 1 mg/L each of chlorite and chlorate and a separate secondary stock solution containing 1 mg/L bromate by performing the appropriate dilutions of the 1000 mg/L stock standards. Calibration standards can then be prepared from the secondary solutions using the appropriate dilutions. Dilute working standards should be prepared monthly, except those that contain chlorite, which must be prepared every two weeks, or sooner if evidence of degradation is indicated by repeated QC failures. Concentration ranges used in this application note are shown in Table 1.

### SAMPLE PREPARATION

For the present analysis, mineral waters B and C were degassed for 10–15 min under vacuum due to an excess amount of bicarbonate in the samples. Increased amounts of bicarbonate in the sample can produce shifts in retention

times as shown in Figures 1A and 1B. In addition, due to the presence of significantly high concentrations of sulfate in mineral water C, the sample was diluted 1:5 with DI water prior to analysis.

### RESULTS AND DISCUSSION

The IonPac AS23 is a high-capacity anion-exchange column specifically designed to be used with carbonate/bicarbonate eluent for the determination of the trace DBPs, chlorite, bromate, and chlorate, together with common inorganic anions, including bromide (precursor to bromate), in drinking waters. To simplify the method and avoid manual eluent preparation, this column can be used with electrolytically generated potassium carbonate that is modified by an Electrolytic pH Modifier (EPM) to automatically generate the carbonate/bicarbonate eluent that is required for analyte separation. The IonPac AS23 column was developed using a unique polymer technology to achieve a capacity of 320 µeq/column, higher than the IonPac AS9-HC column (190 µeq/column) described in EPA Method 300.1. The combination of an optimized selectivity for DBP anions, high anion exchange capacity, and improved selectivity of carbonate from inorganic anions and oxyhalides, makes this column an ideal replacement for the AS9-HC column.

Table 1. Calibration Data, Retention Time Precisions, Peak Area Precisions, and Method Detection Limits For DBP Anions						
IonPac AS19 Column						
Analyte	Range (µg/L)	Linearity (r <sup>2</sup> )	Retention Time <sup>a</sup> RSD (%)	Peak Area RSD (%)	MDL Standard (µg/L)	Calculated MDL (µg/L)
Chlorite	2-50	0.9999	0.04	1.20	1.0	0.18
Bromate	1-25	0.9995	0.03	1.40	2.0	0.31
Chlorate	2-50	0.9999	0.01	0.54	1.0	0.28
IonPac AS23 Column						
Chlorite	10-50	0.9999	0.07	2.20	5.0	1.02
Bromate	5-25	0.9998	0.07	2.63	5.0	1.63
Chlorate	10-50	0.9998	0.11	2.48	9.0	2.05

<sup>a</sup>RSD= relative standard deviation, n = 10 for a standard consisting of 10 ppb bromate and 20 ppb each of chlorite and chlorate.

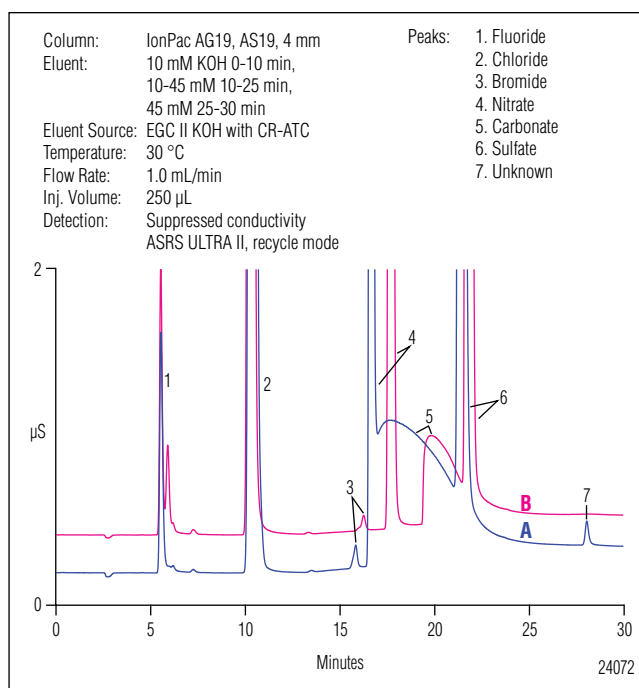


Figure 1. Comparison of mineral water B A) before vacuum degas and B) after vacuum degas.

In this application, we compare the IonPac AS23 column to the hydroxide-selective IonPac AS19 column for the determination of trace DBP anions in natural mineral waters. Figure 2 compares the separation for chlorite, bromate, and chlorate on the IonPac AS19 and AS23 columns. As shown, both columns provide good selectivity for the target DBP anions.

The linear calibration ranges, MDLs, and quality control standard (QCS) performances were evaluated for the hydroxide and carbonate eluent systems. The hydroxide eluent system was calibrated using four increasing concentrations of chlorite and chlorate (2-50  $\mu\text{g/L}$ ) and five increasing concentrations of bromate (1-25  $\mu\text{g/L}$ ). For the carbonate-based system, chlorite and chlorate were calibrated from 10-50  $\mu\text{g/L}$  whereas bromate was calibrated from 5-25  $\mu\text{g/L}$  using three different concentrations. Each system produced a linear response in its respective range with a correlation coefficient greater than 0.999. The improved sensitivity of the hydroxide eluent system, however, allowed a lower minimum reporting limit (MRL) than the carbonate-based system. The MDLs for the target DBPs were determined for each system by performing seven replicate injections of reagent water fortified with the calibration standards at concentrations of three to five times the estimated instrument detection limits.

Table 1 compares the calibration data, retention time and peak area precisions for a QCS, and MDLs for the IonPac AS19 with an electrolytically generated hydroxide eluent to the IonPac AS23 with an electrolytically generated carbonate/bicarbonate eluent. The calculated MDL of bromate with the IonPac AS19 column was 0.31  $\mu\text{g/L}$  compared to 1.63  $\mu\text{g/L}$  using the IonPac AS23 column. This demonstrates that hydroxide eluents improve the sensitivity for bromate compared to carbonate-based eluents and are therefore more suitable to meet the current European regulatory requirement of 3  $\mu\text{g/L}$  bromate in natural mineral waters. Either the AS19 or AS23 based IC systems are capable of measuring the 10  $\mu\text{g/L}$  requirement of bromate for tap water or U.S. bottled water according to the regulations established by the U.S. EPA, U.S. FDA, WHO, and European Commission.

In the U.S., mineral water is defined as water that contains no less than 250 ppm total dissolved solids (TDS) and that originates from a geologically and

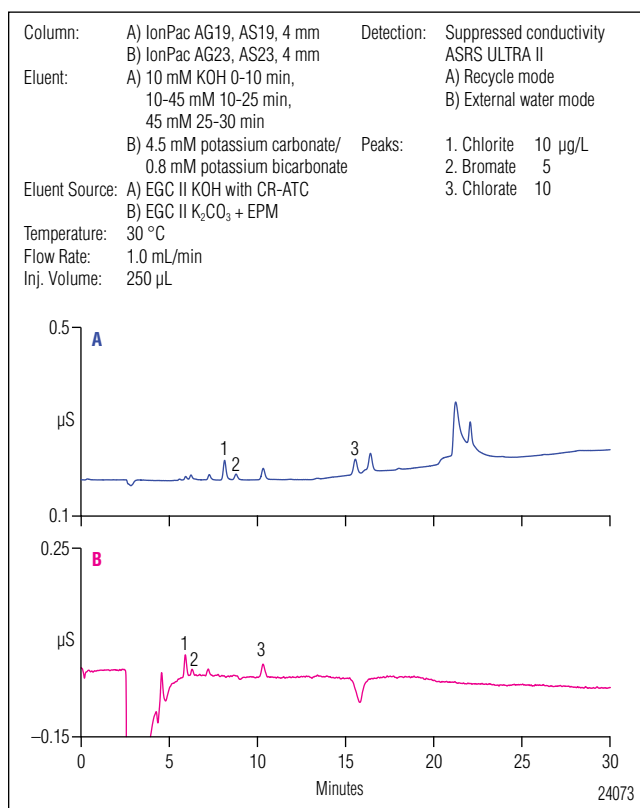


Figure 2. Separation of disinfection byproducts using the A) IonPac AS19 column and B) IonPac AS23 column.

physically protected underground water source. Mineral content must be maintained at a constant level and no minerals may be added to the water.<sup>18</sup> In Europe, mineral water is defined as microbiologically wholesome water, originating from an underground water table or deposit and emerging from a spring tapped at one or more natural or bored exits. It can contain less than 50 ppm TDS.<sup>19</sup> The total mineral content of the waters can vary significantly, with higher mineral concentrations generally appearing in Russia, the Baltic States, and Germany. The differences between regions are most likely a result of differences in the overall compositions of the waters and the geological locations.<sup>20</sup>

In this application, three natural mineral waters from different European countries with TDSs that varied significantly from 136 to 2359 ppm were evaluated. The properties of the investigated water samples are summarized in Table 2. As shown, the ionic strength of mineral water C is significantly higher than observed in typical drinking waters. The absence of bromate in the bottled mineral waters analyzed indicated that ozonation was not used for disinfection.

Tables 3 and 4 summarize typical recoveries for single-operator data obtained using the IonPac AS19 and AS23 columns, respectively, for trace concentrations of DBP anions in three European natural mineral water samples. As shown, chlorite and bromate were not detected in any of the samples analyzed, whereas only a trace concentration of chlorate was detected in mineral water A. To determine the accuracy of the method, the samples were spiked with 5 µg/L bromate and 10 µg/L each of chlorite and chlorate. Calculated recoveries for the spiked mineral water samples were in the range of 86–97% and 84–111% using the IonPac AS19 and AS23 columns, respectively. The analyte recoveries using either a hydroxide or carbonate/bicarbonate eluent were within the acceptable range of 75–125% according to the criteria described in EPA Method 300.1. Figure 3 compares chromatograms of mineral water A using the IonPac AS19 and AS23 columns. Figure 4 shows the same chromatograms spiked with 5 µg/L bromate and 10 µg/L each of chlorite and chlorate, which resulted in good recoveries for both eluents. Although bromide was not quantified in this study, the estimated concentrations were approximately 16 µg/L in mineral waters A and B and 2 µg/L in mineral water C. Therefore, ozonation of mineral waters A and B could potentially produce bromate. To demonstrate the applicability of detecting bromate at concentrations significantly less than the 3 µg/L European regulatory limit for ozonated mineral waters, mineral water A was spiked with 0.5 µg/L bromate (Figure 5). As shown, bromate can be observed easily at this concentration, with good peak-to-peak baseline noise of 0.3–0.5 nS.

**Table 2. Concentrations in mg/L of Cations and Anions in the Investigated Mineral Water Samples**

Mineral water	Na <sup>+</sup>	K <sup>+</sup>	Mg <sup>2+</sup>	Ca <sup>2+</sup>	F <sup>-</sup>	Cl <sup>-</sup>	NO <sub>3</sub> <sup>-</sup>	HCO <sub>3</sub> <sup>-</sup>	SO <sub>4</sub> <sup>2-</sup>
A	11.8	6.2	8	11.5	— <sup>a</sup>	13.5	6.3	71	8.1
B	4.5	0.5	8	32.0	— <sup>a</sup>	5.0	<2	133	7.0
C	4.2	— <sup>a</sup>	117	510	1.8	3.0	<0.1	278	1445

<sup>a</sup>Not specified.

**Table 3. Recoveries of Disinfection Byproduct Anions in Natural Mineral Waters Using the IonPac AS19 Column**

Mineral water	Analyte	Amount found (µg/L)	Amount added (µg/L)	Recovery (%)
A	Chlorite	<MDL	10	87.7
	Bromate	<MDL	5.0	96.0
	Chlorate	4.4	10	91.1
B	Chlorite	<MDL	10	86.4
	Bromate	<MDL	5.0	97.4
	Chlorate	<MDL	10	90.7
C	Chlorite	<MDL	10	87.6
	Bromate	<MDL	5.0	94.7
	Chlorate	<MDL	10	92.8

**Table 4. Recoveries of Disinfection Byproduct Anions in Natural Mineral Waters Using the IonPac AS23 Column**

Mineral water	Analyte	Amount found (µg/L)	Amount added (µg/L)	Recovery (%)
A	Chlorite	<MDL	10	107.6
	Bromate	<MDL	5.0	91.2
	Chlorate	4.6	10	99.3
B	Chlorite	<MDL	10	110.6
	Bromate	<MDL	5.0	93.5
	Chlorate	<MDL	10	92.9
C	Chlorite	<MDL	10	104.3
	Bromate	<MDL	5.0	83.9
	Chlorate	<MDL	10	102.6

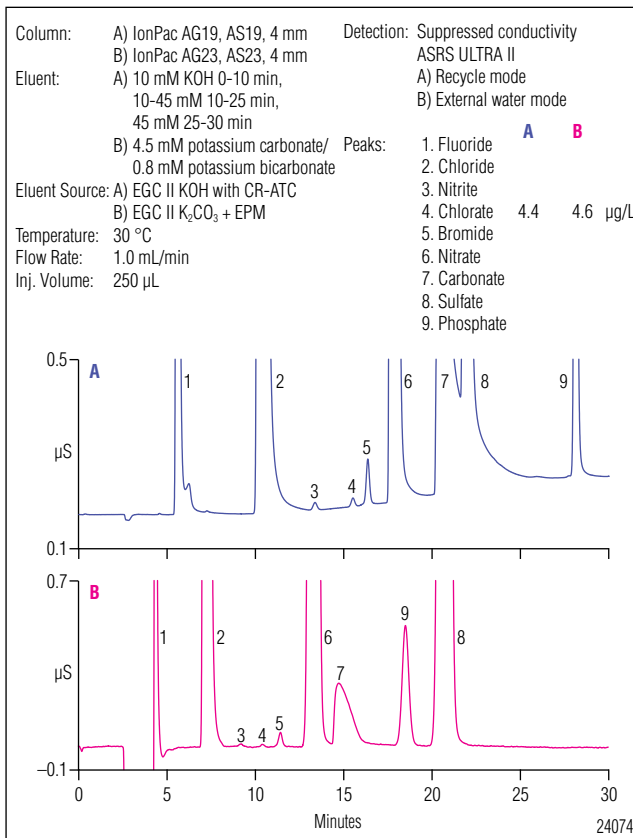


Figure 3. Comparison of the A) IonPac AS19 and B) IonPac AS23 columns for the separation of DBP anions in mineral water A.

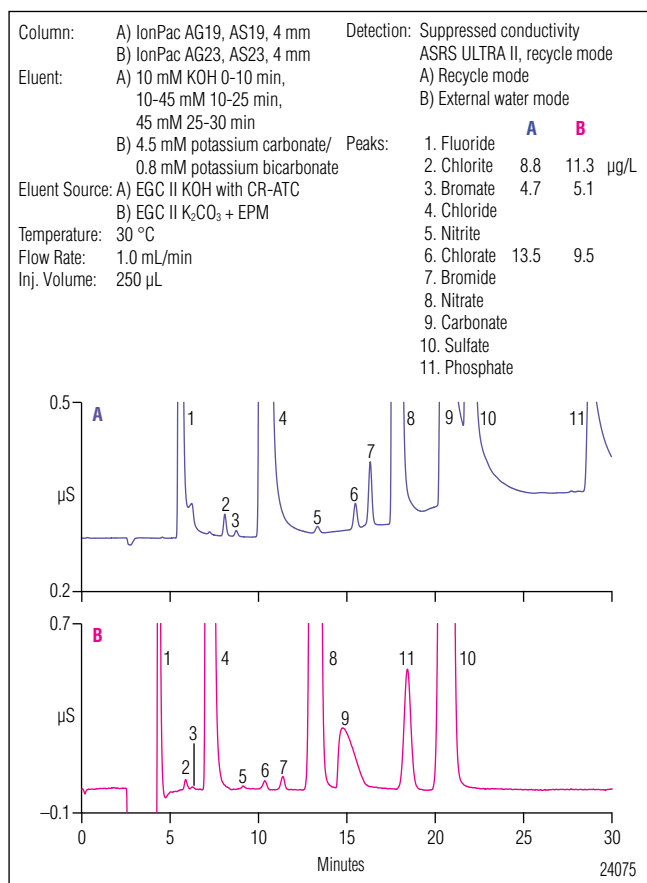


Figure 4. Comparison of the A) IonPac AS19 and B) IonPac AS23 columns for the separation of trace concentrations of common anions and DPB anions spiked in mineral water A.

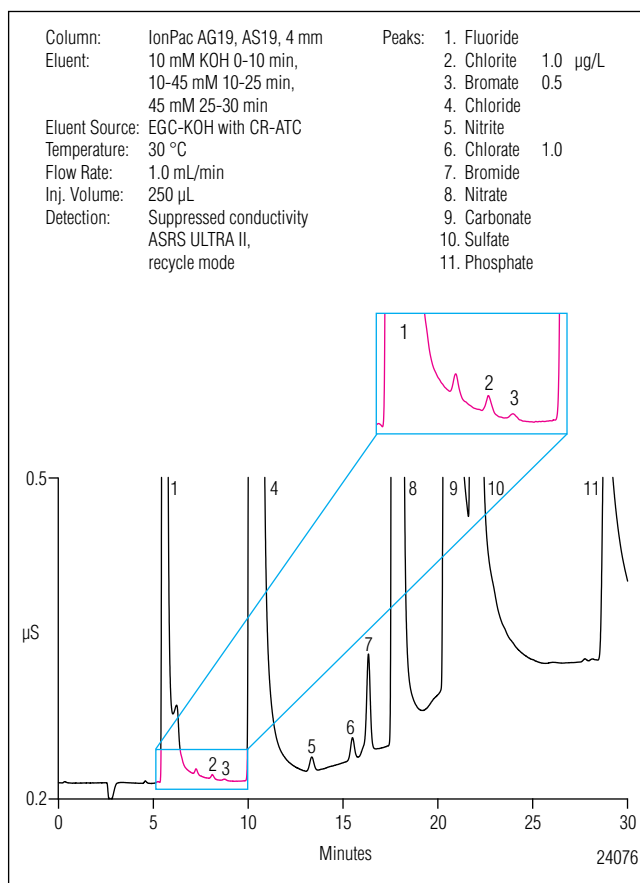


Figure 5. Chromatogram of mineral water A spiked with 1 µg/L each chlorite and chlorate and 0.5 µg/L bromate.

## CONCLUSION

The IonPac AS19 column using an electrolytically generated hydroxide eluent was compared to the AS23 column using an electrolytically generated carbonate/bicarbonate eluent for the determination of trace concentrations of DBP anions in natural mineral waters. The improved sensitivity using a hydroxide eluent allowed the detection of lower concentrations of bromate, a potential human carcinogen, in drinking waters. Therefore, the IonPac AS19 with an electrolytically generated hydroxide eluent is recommended for laboratories that must comply with EU Directive 2003/40/EC, which permits a maximum of 3 µg/L bromate in mineral waters treated with ozone. The use of

either the IonPac AS19 column with a hydroxide eluent or IonPac AS23 column with a carbonate/bicarbonate eluent provides the required sensitivity to meet the maximum permissible limit of 10 µg/L bromate currently required by most regulatory agencies. Both columns demonstrated good resolution between bromate and chloride and comparable recovery for mineral water samples spiked with known concentrations of chlorite, bromate, and chlorate. In addition, hydroxide or carbonate/bicarbonate eluents can be generated on-line from deionized water, freeing the operator from manually preparing eluents. This increases the automation, ease-of-use, and reproducibility between analysts and laboratories.



---

## REFERENCES

1. Rodwan, J.G. Reprint from *The Bottled Water Reporter*, Aug/May 2005, available at <http://www.beveragemarketing.com/news3e.htm>.
2. U.S. EPA, *Water Health Series: Bottled Water Basics*, U.S. Environmental Protection Agency, Cincinnati, OH, Sept 2005.
3. U.S. EPA, Occurrence Assessment for the Final Stage 2 Disinfectants and Disinfection Byproducts Rule, Document No. 815-R-05-011, U.S. Environmental Protection Agency, Cincinnati, OH, December 2005.
4. World Health Organization, International Programme on Chemical Safety-Environmental Health Criteria 216, *Disinfectants and Disinfection By-Products*, Geneva, Switzerland, 2000.
5. Thompson, K.C.; Guinamant, J.L.; Elwaer, A.R.; McLeod, C.W.; Schmitz, F.; De Swaef, G.; Quevauviller, P. Interlaboratory Trial to Determine the Analytical State-of-the-Art of Bromate Determination in Drinking Water. *J. Environ. Monit.*, **2000**, 2, 416-419.
6. Wagner, H.P.; Pepich, B.V.; Hautman, D.P.; Munch, D.J. Analysis of 500 ng/L Levels of Bromate in Drinking Water by Direct Injection Suppressed Ion Chromatography Coupled with a Single, Pneumatically Delivered Post-Column Reagent. *J. Chromatogr. A*, **1999**, 850, 119-129.
7. US EPA. National Primary Drinking Water Regulations: Disinfectants and Disinfection Byproducts. *Fed. Regist.* **1998**, 63 (241), 69389-69476.
8. European Parliament and Council Directive No. 98/83/EC, *Quality of Water Intended for Human Consumption*, 1998.
9. World Health Organization, *Bromate in Drinking Water*—Background Document for the Development of WHO Guidelines for Drinking Water Quality, 2005.
10. Food and Drug Administration. Beverages: Bottled Water. *Fed. Reg.* **2001**, 66 (60), 16858-16868.
11. European Parliament and Council Directive No. 2003/40/EC, *Establishing the List, Concentration Limits and Labeling Requirements for the Constituents of Natural Mineral Waters and the Conditions for Using Ozone-Enriched Air for the Treatment of Natural Mineral Waters and Spring Waters*, 2003.
12. Hautman, D. P.; Munch, D. J. Method 300.1: Determination of Inorganic Anions in Drinking Water by Ion Chromatography. U. S. Environmental Protection Agency, Cincinnati, OH, 1997.
13. US EPA. National Primary Drinking Water Regulations: Stage 2 Disinfectants and Disinfection By-products Rule. *Fed. Reg.* **2006**, 71 (2), 388.
14. Wagner, H. P.; Pepich, B. V.; Hautman, D. P.; Munch, D. J. Method 317.0, rev 2: Determination of Inorganic Oxyhalide Disinfection Byproducts in Drinking Water Using Ion Chromatography with the Addition of a Postcolumn Reagent for Trace Bromate Analysis. U. S. Environmental Protection Agency, Cincinnati, OH, 2001.
15. Wagner, H. P.; Pepich, B. V.; Hautman, D. P.; Munch, D. J.; Salhi, E.; von Gunten, U. Method 326.0: Determination of Inorganic Oxyhalide Disinfection By-Products in Drinking Water Using Ion Chromatography Incorporating the Addition of a Suppressor Acidified Postcolumn Reagent for Trace Bromate Analysis. U. S. Environmental Protection Agency, Cincinnati, OH, 2001.
16. Creed, J. T.; Brockhoff, C. A.; Martin, T. D. Method 321.8: Determination of Bromate in Drinking Waters by Ion Chromatography Inductively Coupled Plasma–Mass Spectrometry. U.S. Environmental Protection Agency, Cincinnati, OH, 1997.
17. Dionex Corporation. Determination of Trace Concentrations of Oxyhalides and Bromide in Municipal and Bottled Waters Using a Hydroxide-Selective Column with a Reagent-Free Ion Chromatography System. Application Note 167, LPN 1662; Sunnyvale, CA 2004.
18. Dionex Corporation. Determination of Trace Concentrations of Disinfection By-Product Anions and Bromide in Drinking Water Using Reagent-Free™ Ion Chromatography Followed by Postcolumn Addition of o-Dianisidine for Trace Bromate Analysis. Application Note 168, LPN 1706; Sunnyvale, CA 2004.

19. Dionex Corporation. Determination of Disinfection By-Product Anions and Bromide in Drinking Water Using a Reagent-Free Ion Chromatography System Followed by Postcolumn Addition of an Acidified On-Line Generated Reagent for Trace Bromate Analysis. Application Note 171, LPN 1767; Sunnyvale, CA 2006.
20. Posnick, L.M.; Kim, H. Bottled Water Regulation and the FDA. *Food Safety Magazine*, Aug/Sept **2002**, 7(13-15).
21. European Parliament and Council Directive No. 80/777/EEC, The Approximation of the Laws of the Member States Relating to the Exploitation and Marketing of Natural Mineral Waters, 1980.
22. Misund, A.; Frengstad, B.; Siewers, U.; Reimann, C. Variation of 66 Elements in European Bottled Mineral Waters. *Sci. Total Environ.* **1999**, 243/244, 21-41.

Reagent-Free and RFIC are trademarks and AutoSuppression, ASRS, Chromeleon, EluGen, and IonPac are registered trademarks of Dionex Corporation.

Passion. Power. Productivity.



**Dionex Corporation**

1228 Titan Way  
P.O. Box 3603  
Sunnyvale, CA  
94088-3603  
(408) 737-0700

**North America**

U.S. (847) 295-7500  
Canada (905) 844-9650

**South America**

Brazil (55) 11 3731 5140

**Europe**

Austria (43) 1 616 51 25 Benelux (31) 20 683 9768 (32) 3 353 4294  
Denmark (45) 36 36 90 90 France (33) 1 39 30 01 10 Germany (49) 6126 991 0  
Ireland (353) 1 885 1700 Italy (39) 02 51 62 1267 Switzerland (41) 62 205 9966  
United Kingdom (44) 1276 691722

**Asia Pacific**

Australia (61) 2 9420 5233 China (852) 2428 3282 India (91) 22 28475235  
Japan (81) 6 6885 1213 Korea (82) 2 2653 2580 Singapore (65) 6289 1190

[www.dionex.com](http://www.dionex.com)



LPN 1890 PDF 03/07  
©2007 Dionex Corporation